

# 8. Methods in Developing Mobile Phase Condition for C<sub>18</sub> Column

## Introduction

In reversed phase HPLC, octadecyl group bonded silica columns (C<sub>18</sub>, ODS) are the most widely employed. A proper mobile phase condition for C<sub>18</sub> columns can be achieved by referring to publications, application notes from manufactures and your own experiences. This section shows traditional methods of developing mobile phase condition. The following columns are used as examples because of their popularity.

Packing material : COSMOSIL 5C<sub>18</sub>-MS-II, COSMOSIL 5C<sub>18</sub>-AR-II  
 Column size (I.D. x length) : 4.6 mm I.D x 150 mm


## Methods for Developing Mobile Phase Conditions

In the Isocratic method, the mobile phase composition remains constant throughout the run. In the gradient method, the mobile phase composition changes. Each method needs strict preparation of the mobile phase and control of the column temperature to achieve good separation.

### • Isocratic Method

Methods for developing mobile phase condition generally proceed as follows. First, elute the samples with strong solvents to check whether the samples can be detected. Then, separate the samples by controlling the retention time through changing the mobile phase condition. Increasing the concentration of strong elution efficiency solvents results in shorter retention time and decreasing in concentration of them results in longer retention time. If your samples are ionizable, such as acid and amine group, pH control with buffers is highly advisable. The ionization control method or ion-pair chromatography is used to increase the retention of ionized samples. The method uses ion-pair reagents (e.g., alkyl benzene sulfonate for basic compounds, quaternary ammonium for acidic compounds) into in the mobile phase to form ion pairs with samples.

(e.g.,) Procedures for Basic Condition Setting

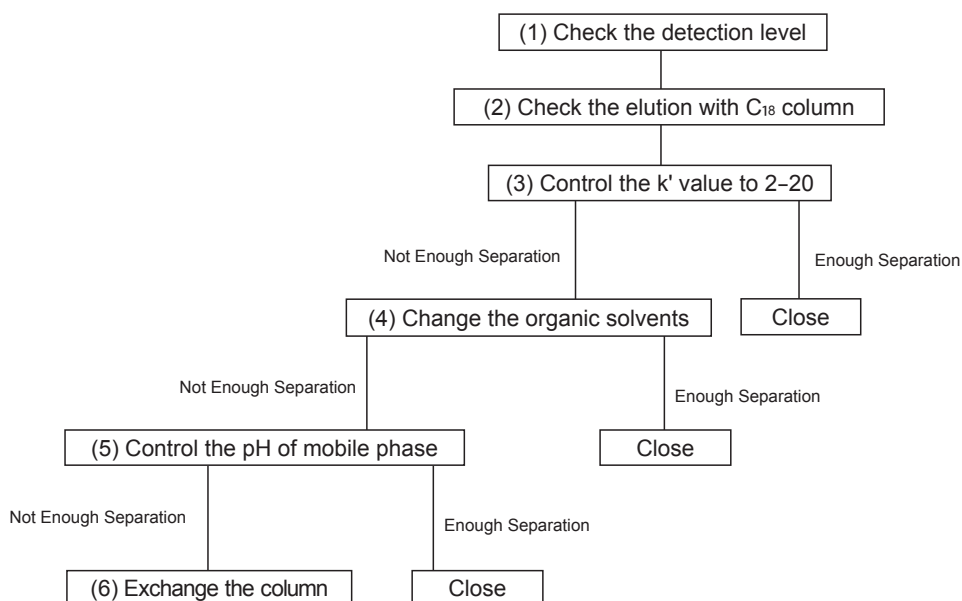

I. HPLC Columns

II. UHPLC Columns

III. Preparative Packing Materials

IV. Related Products

V. Applications

VI. Technical Notes

VII. Index

1. Check the detection of samples with strong elution solvents. In this step, check the detection by connecting the injector directly to the detector without a column.
2. Consult references and carbon numbers and check the elution with C<sub>18</sub> column using aqueous mobile phase with methanol.
3. Control the k' value to 2–20 by changing the amount of the methanol in the mobile phase.
4. If the separation is not enough, change the methanol to acetonitrile or add tetrahydrofuran to change the selectivity.
5. If tailing peaks occur for basic compounds, control the pH by adding buffers to the mobile phase.
6. If separation is not satisfactory after step 5, change the column to other C<sub>18</sub> columns or columns with different stationary phases such as alkyl-based, aromatic-based and others.

- **Gradient Method**

Gradient method changes organic solvent composition continuously in the mobile phase. It is useful for shortening the separation time of samples with wide range of hydrophobicity and molecular weight, with long elution time, and with great changes in retention time by slight changes in organic solvent composition. It is also useful for large molecule weight compounds like peptides. Gradient method is not compatible with RI detector. Gradient method development is beyond the scope that can be discussed here.


## Easy Method to Set the Reversed Phase Condition

Reversed phase chromatography does not have an easy method to set mobile phase conditions, unlike normal phase chromatography mobile phase conditions that can simply be determined by thin layer chromatography. Therefore, the composition of the mobile phase (concentration of organic solvent) is often determined by repeated trial and error. If you know the structure of the analytes, here is a general instruction on configuring an appropriate mobile phase organic solvent concentration.

Suitable concentration of organic solvent for basic chemical skeleton + effects from substituents  
= The best organic solvent concentration

### ● Condition Setting

Select the condition based on retention time of the basic chemical skeleton shown in Figure 1, then adjust for the effect of hetero atom and substituents.

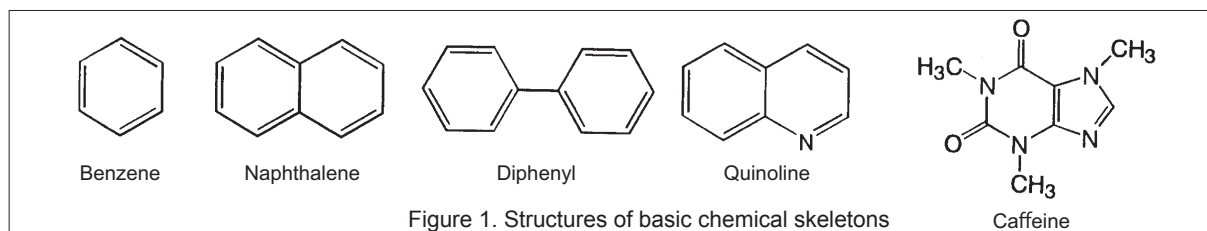

1. Select the best concentration of organic solvent with its corresponding basic chemical skeleton. \*Refer Table 1

2. Adjust the concentration of the organic solvent considering effect of hetero atom. \*Refer Table 2

3. Adjust the concentration of organic solvent considering the effects from substituents. \*Refer Table 3

Contain dissociate substituent

No dissociate substituent

4. Adjust the concentration of the organic solvent considering effects from dissociable substituent.

Complete

Complete

1. Choose a compound of similar basic chemical structure as the target sample in Figure 1. Select the best organic solvent concentration.

Table 1. Retention time of the basic chemical skeleton

Basic skeleton	Column	Retention Time Under Different Methanol Concentrations (min)						
		80%	70%	60%	50%	40%	30%	20%
Benzene	5C <sub>18</sub> -MS-II	-	4	7	11	20	-	-
	5C <sub>18</sub> -AR-II	-	4	7	13	23	-	-
Naphthalene	5C <sub>18</sub> -MS-II	5	8	18	-	-	-	-
	5C <sub>18</sub> -AR-II	5	10	22	-	-	-	-
Diphenyl	5C <sub>18</sub> -MS-II	8	13	-	-	-	-	-
	5C <sub>18</sub> -AR-II	7	15	-	-	-	-	-
Quinoline	5C <sub>18</sub> -MS-II	-	-	-	-	6	11	-
	5C <sub>18</sub> -AR-II	-	-	-	-	8	17	-
Caffeine	5C <sub>18</sub> -MS-II	-	-	-	-	-	4	9
	5C <sub>18</sub> -AR-II	-	-	-	-	-	4	9

Column: COSMOSIL 4.6 mm I.D. × 150 mm Flow Rate: 1.0 ml/min Detection: UV 254 nm

2. Adjust the organic solvent concentration considering effect of hetero atom as shown in Table 2.

Table 2. Organic solvent concentration adjustment from hetero rings or polycyclic aromatics

Hetero Rings, polycyclic Aromatics		Sample	5C <sub>18</sub> -MS-II	5C <sub>18</sub> -AR-II
1 of Conjugate Ring		Benzene	+10%	+10%
Heterocyclic Hetero Atom	1 of S	Thiophene	±0%	±0%
	1 of O	Furane	-5%	-5%
	1 of N	Pyridine	-20%	-10%
1 of Carbonyl Group		Quinone	-5%	-5%
1 of Double Bond		-	-5%	-5%

3. Adjust the concentration of organic solvent considering effect from substituents as shown in Table 3.

Table 3. Organic solvent concentration adjustment from substituents

Substituent	Methanol Concentration		Substituent	Methanol Concentration
	5C <sub>18</sub> -MS-II	5C <sub>18</sub> -AR-II		
-F	0	0	-CH <sub>2</sub> - (Alkyl-chain) MeOH concentration of basic skeleton	100-90% +10% (4 of -CH <sub>2</sub> -) 90-80% +10% (3 of -CH <sub>2</sub> -) 80-60% +10% (2 of -CH <sub>2</sub> -) < 60% +10% (1 of -CH <sub>2</sub> -)
-Cl	+10%	+10%		
-Br	+10%	+10%		
-I	+20%	+15%		
-CONH <sub>2</sub>	-40%	-40%		
-COCH <sub>3</sub>	-10%	-10%		
-COOCH <sub>3</sub>	0	0	-Phenyl MeOH concentration of basic skeleton	100-90% +5% (1 of - Phenyl) 90-60% +10% (1 of - Phenyl) < 60% +20% (1 of - Phenyl)
-OCH <sub>3</sub>	0	0		
-CHCH <sub>2</sub> O	-10%	-10%		
-CH <sub>2</sub> OH	-30%	-30%		
-OH	-30%	-30%		
-NO <sub>2</sub>	-10%	-5%		
-CN	-20%	-15%		
-NH <sub>2</sub>	-40%	-30%		
-SCH <sub>3</sub>	+10%	+10%		

Column: COSMOSIL 4.6 mm I.D. × 150 mm

Flow Rate: 1.0 ml / min Detection: UV 254 nm

\* Effect may shift somewhat by the position of the substituent.

4. Compounds with a dissociative substituent are extremely sensitive toward slight pH change. Maintain consistent mobile phase pH to obtain reproducible data. Table 4 shows the influence of acidic (pH 2) and neutral (pH 7) substituents to the retention.

Table 4. Effect of dissociate substituent to organic solvent

Dissociable Substituent	Change of Methanol Concentration (pH 2)	Change of Methanol Concentration (pH 7)
-COOH	-10~-20%	-30~-40%
-SO <sub>3</sub> H	-20~-40%	-30~-40%
-PO <sub>4</sub> H <sub>2</sub>	-20%	-50%
-BO <sub>2</sub> H <sub>2</sub>	-20%	-20%
-NH <sub>2</sub> (molecular type)	-60%	-10%
-NH <sub>2</sub> (cyclic amine)	-50~-60%	-10~-20%
-NH <sub>2</sub> (ionic type)	-	-40~-50%

Column :COSMOSIL 5C<sub>18</sub>-MS-II, 4.6 mm I.D. x 150 mm  
Buffer pH2 :20mmol/l H<sub>3</sub>PO<sub>4</sub>  
pH7 :20mmol/l H<sub>3</sub>PO<sub>4</sub>/Na<sub>2</sub>HPO<sub>4</sub>=2/3  
Flow Rate :1.0 ml/min  
Detection :UV 254 nm

# Technical Information

## ● Example of Condition Setting

Column: COSMOSIL 5C<sub>18</sub>-MS-II 4.6 mm I.D. × 150 mm

### (1) 5-Benzyloxyindole

<Calculation> Basic skeleton Naphthalene like + (hetero ring N)  
 =70%+ (-20%)  
 =50%  
 Substituent (Phenyl) + (-OCH<sub>2</sub>- is equal to -OCH<sub>3</sub>)  
 =(+10%) + (+0%)  
 Basic skeleton + Substituent = 50% + (+10%) = 60%  
 <Result> 60%Methanol (Methanol:Water=60:40)  
 Retention time=13.7 min

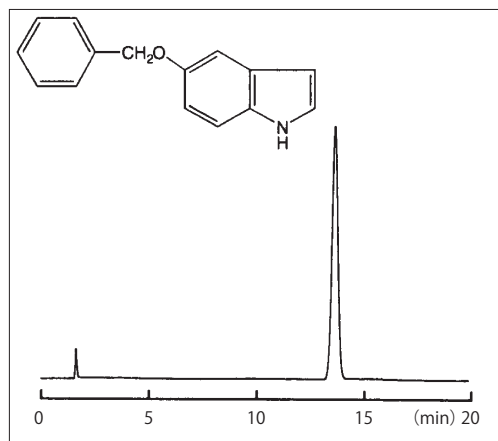


Figure 2. Analysis of 5-Benzyloxyindole

### (2) Homovanillic Acid

<Calculation> Basic skeleton Benzene=60%  
 Nondissociative substituent (-OH) + (-OCH<sub>3</sub>) + (-CH<sub>2</sub>)  
 =(-30%) + (0%) + (+10%)  
 = -20%  
 Dissociable substituent -COOH = -10~-20% (pH 2)  
 -30~-40% (pH 7)  
 Basic skeleton + Substituent = Methanol concentration is  
 Acid range (pH 2) 30-20%  
 Neutral range (pH 7) 10-0%  
 <Result> (pH2) 30%Methanol : Retention time=5.7 min  
 20%Methanol : Retention time=11.7 min  
 (pH7) 10%Methanol : Retention time=4.0 min  
 0%Methanol : Retention time=12.1 min

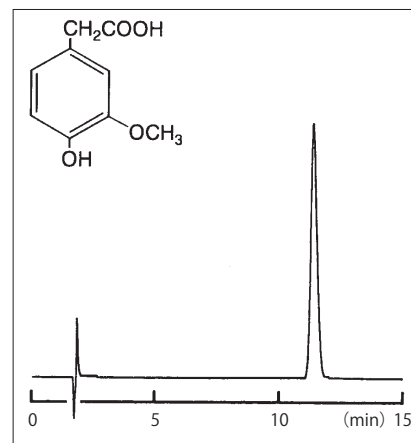


Figure3. Analysis of 20% Methanol (pH 2)

\* Actual retention prediction results may have ±10% error in organic solvent concentration calculated.